






**(DARK = OXYGENATED BLOOD)**  
**(LIGHT = DEOXYGENATED BLOOD)**

**FIG. 1A.**

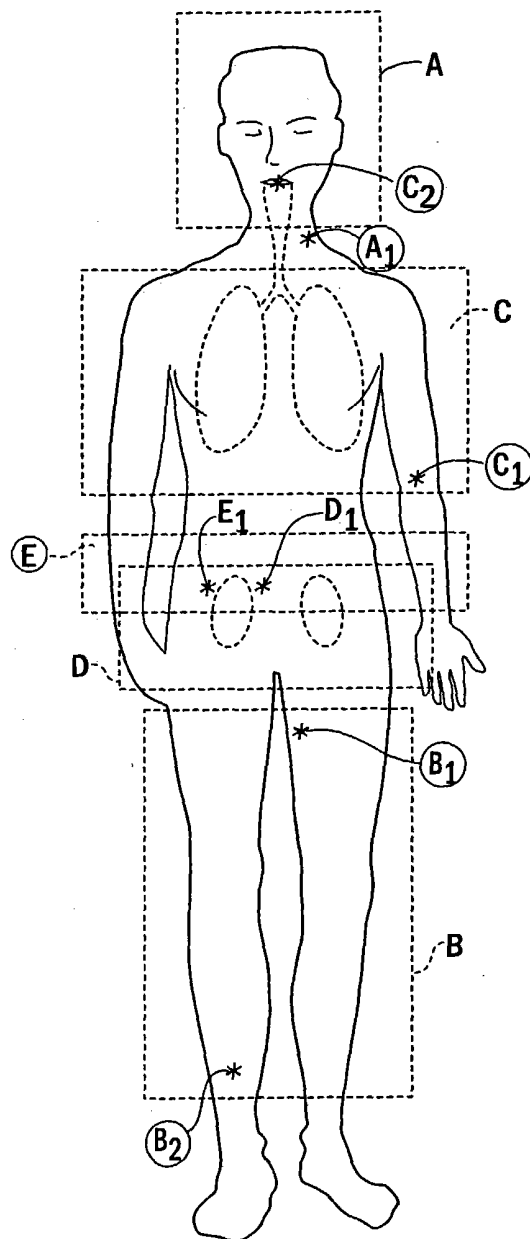


**FIG. 1B.**

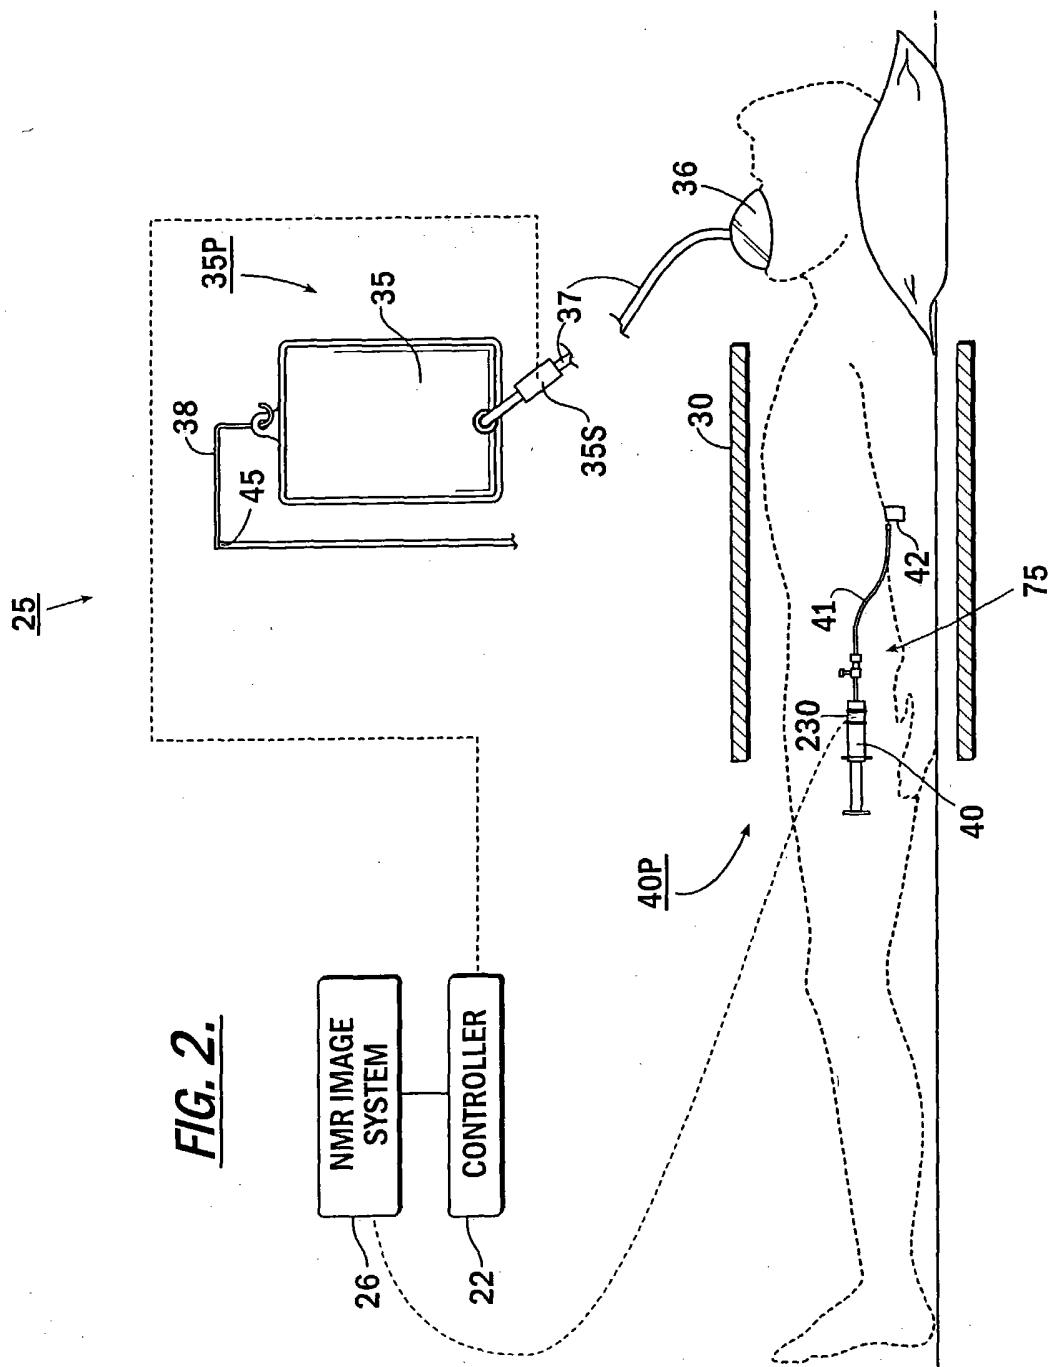


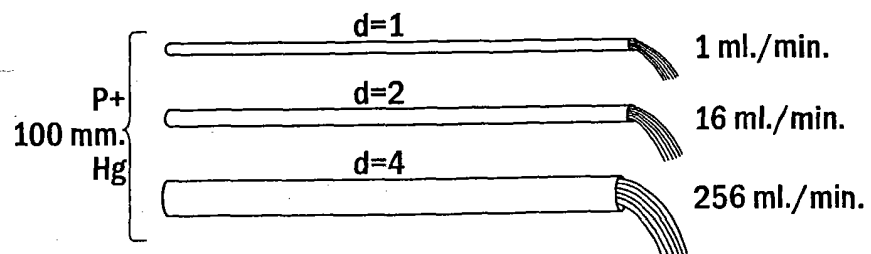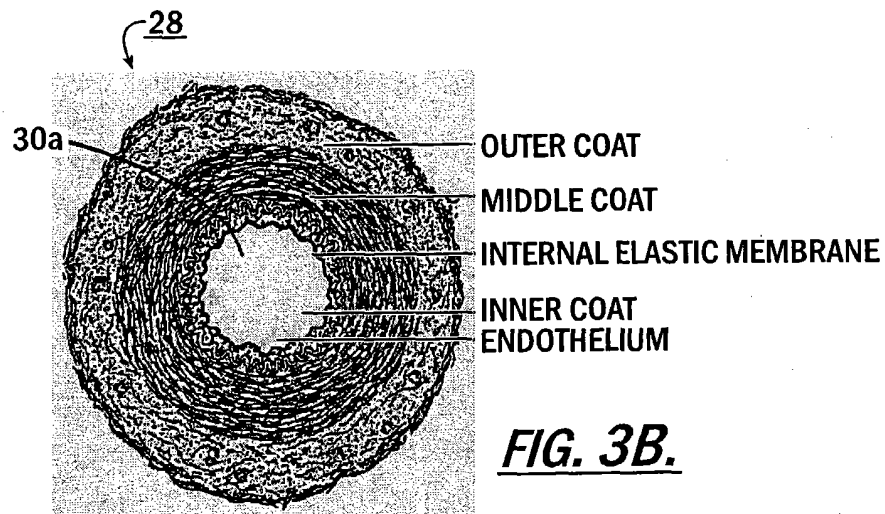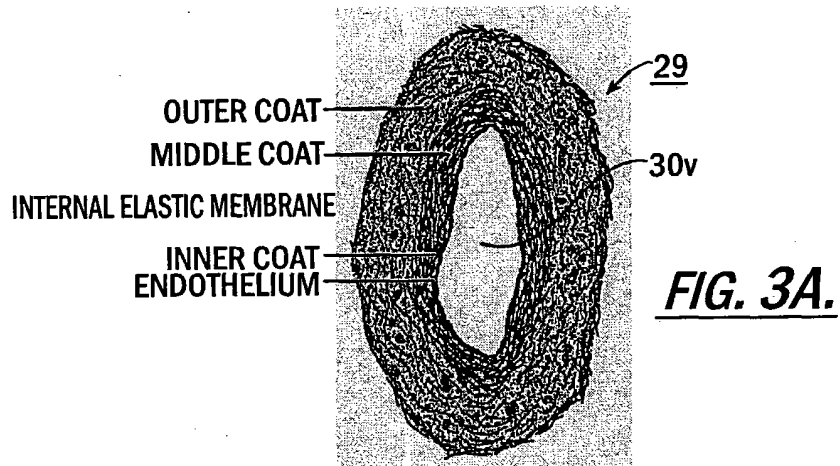


**FIG. 4.**

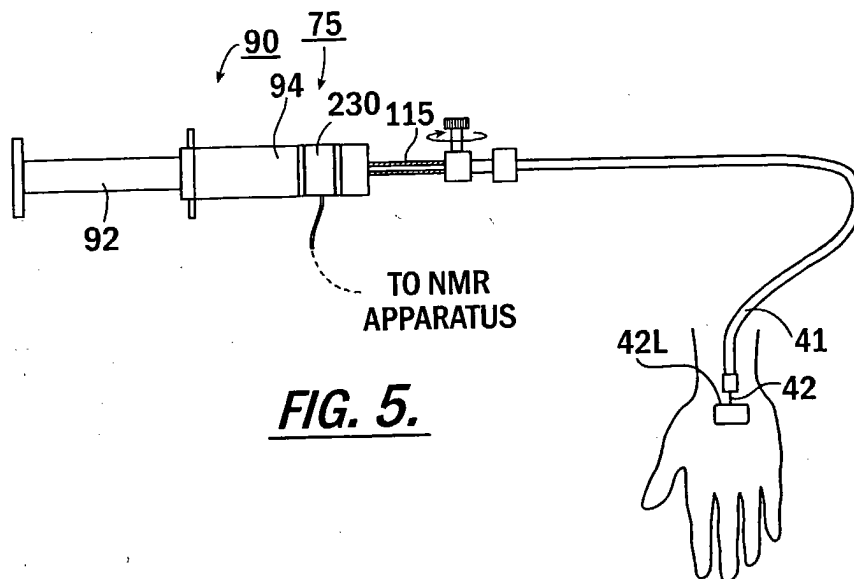


**FIG. 5.**

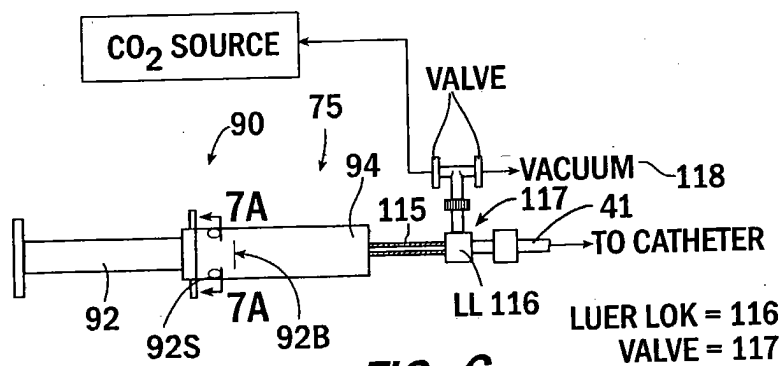



**FIG. 6.**







**FIG. 7A.**

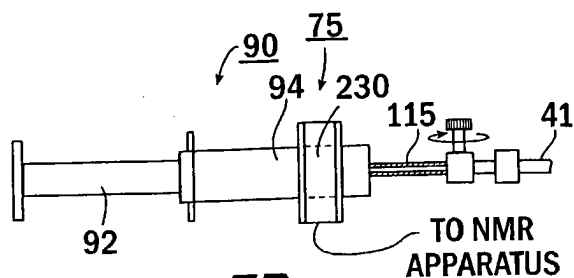

**FIG. 7B.**

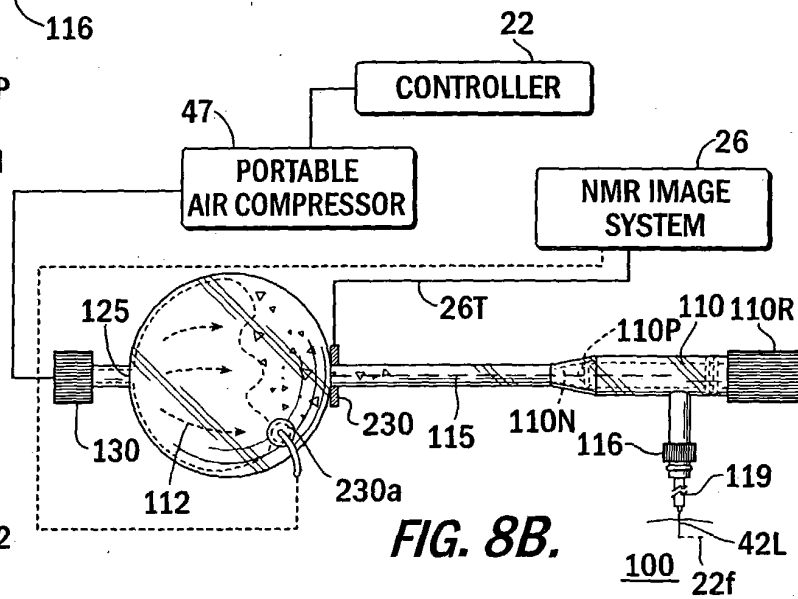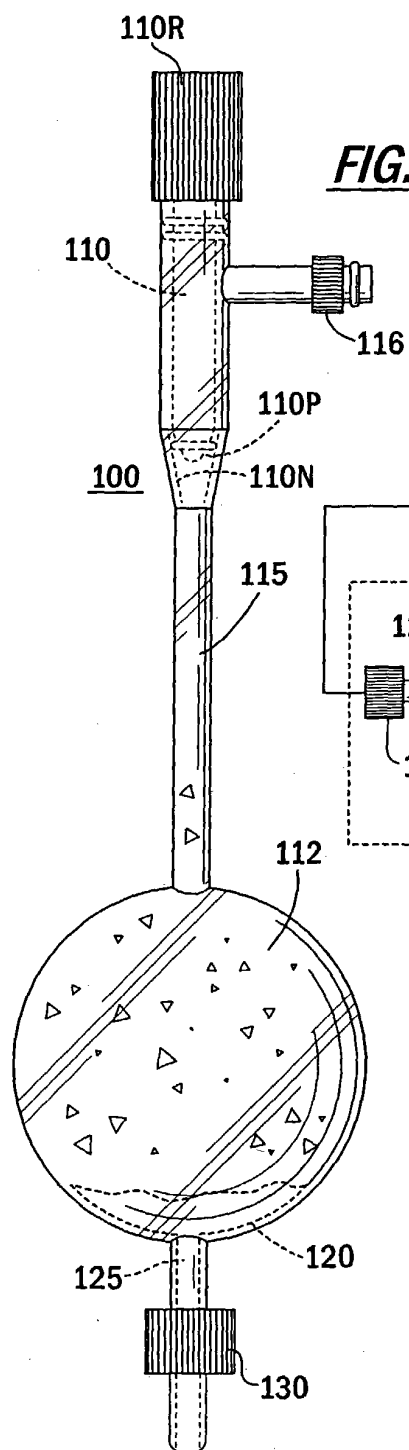
**FIG. 8A.**

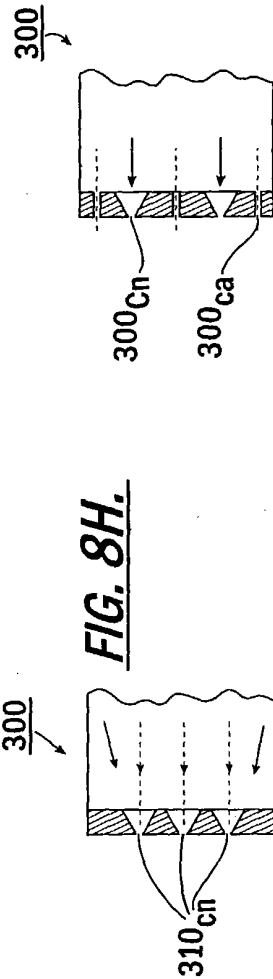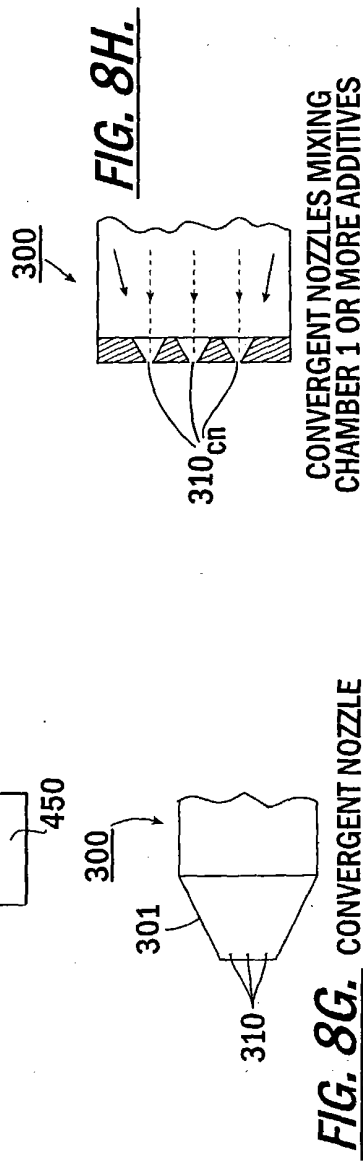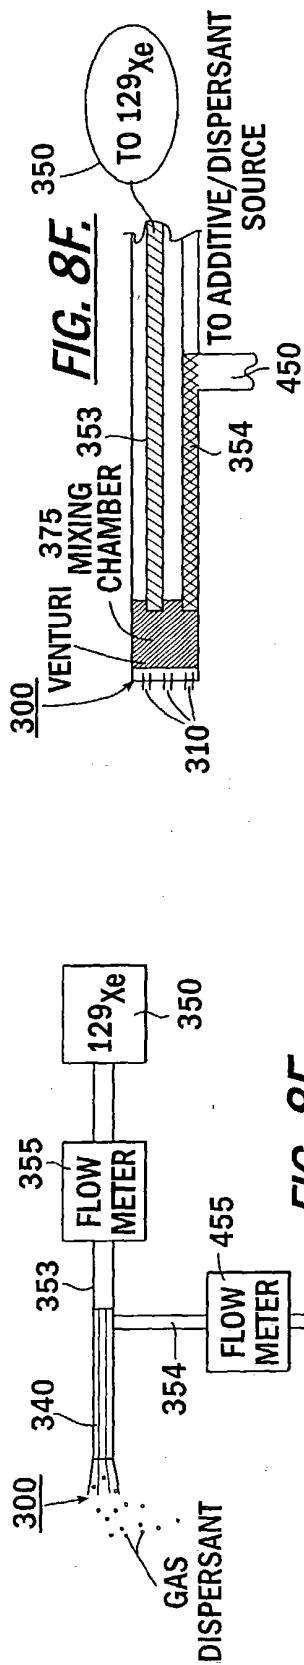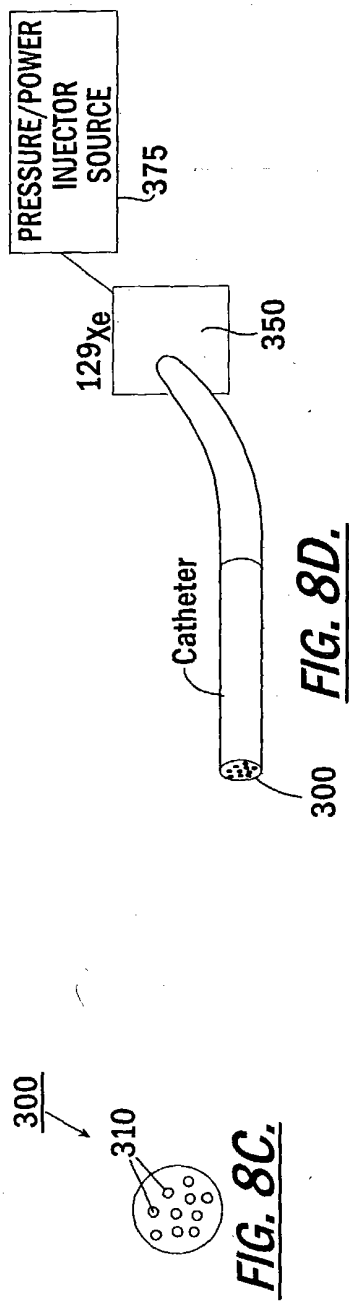

**FIG. 8G.** CONVERGENT NOZZLE







CONVERGENT NOZZLES MIXING CHAMBER 1 OR MORE ADDITIVES

**FIG. 8I.**

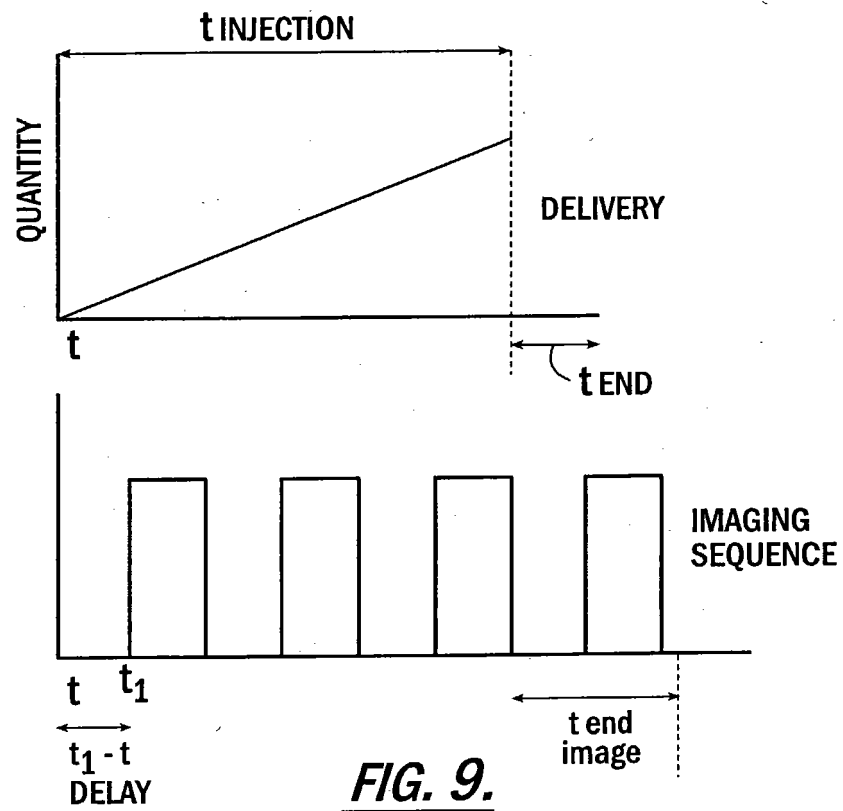


**FIG. 9.**

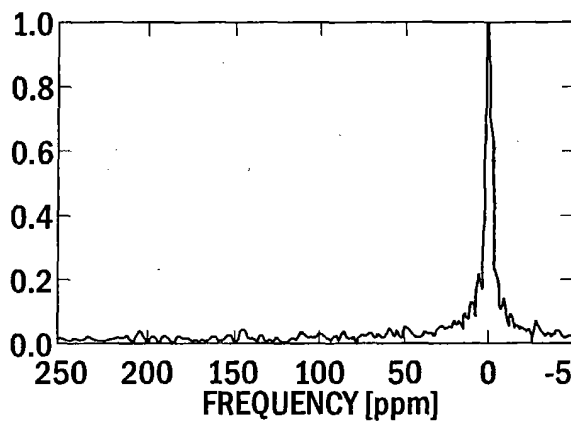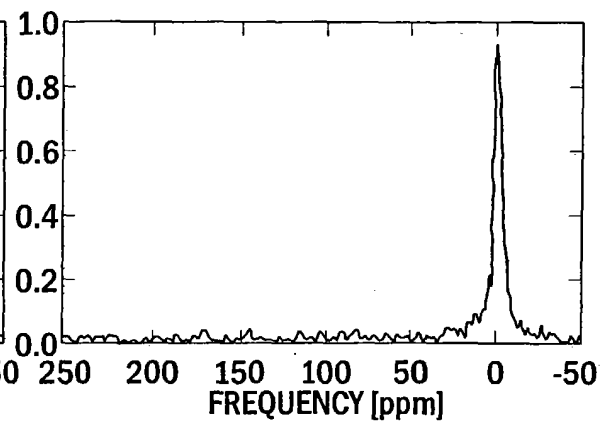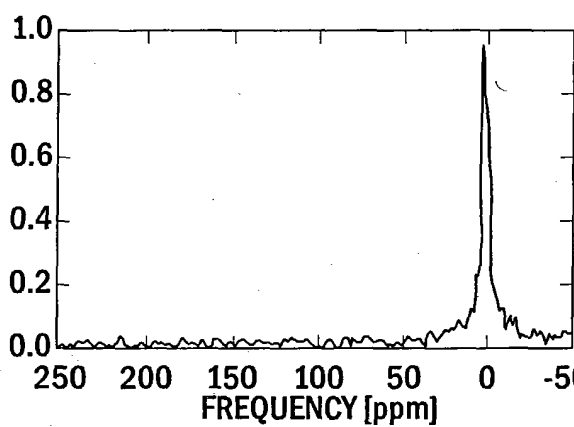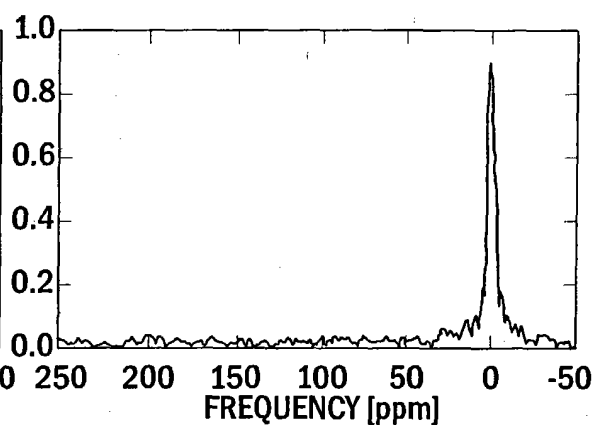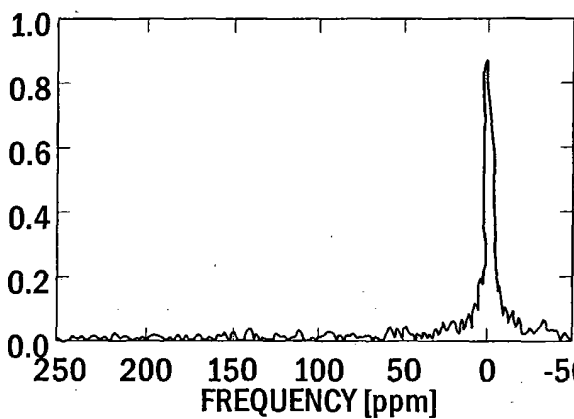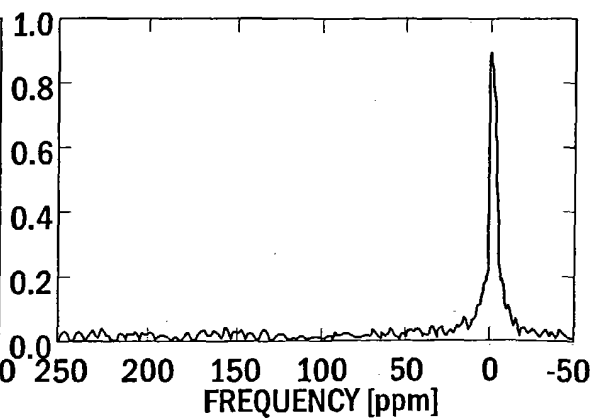


FIG. 10A.FIG. 10B.FIG. 10C.FIG. 10D.FIG. 10E.FIG. 10F.

10/10

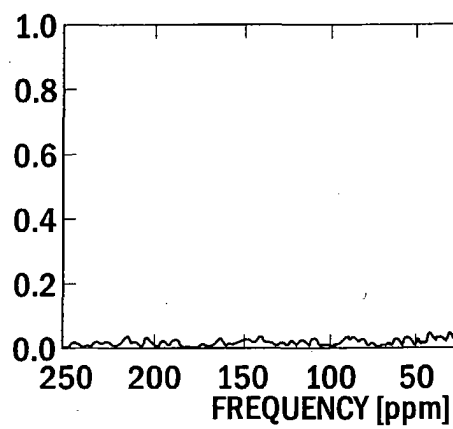

**FIG. 10G.**

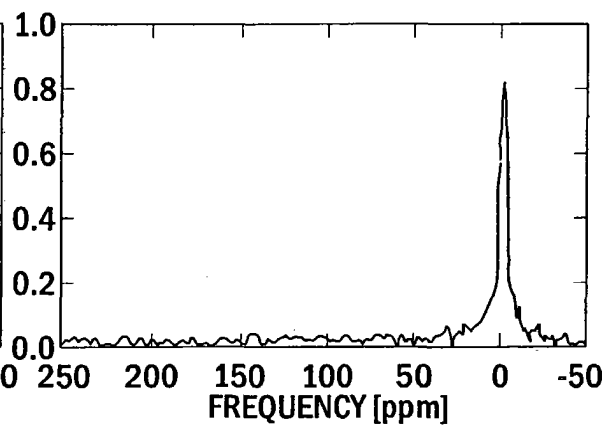

**FIG. 10H.**